

Bertin Pharma also markets preanalytical products, EIA kits, antibodies, CVP450s & biochemicals for:

- Cardiology / Hypertension
- Diabetes / Obesity
- Endocrinology / Metabolism
- **▶** Inflammation
- Pharmacology
- Psychopharmacology
- Nitric Oxide
- Oncology / Apoptosis
- Oxidative injury
- Cell signaling
- Drug metabolism

Do not hesitate to contact our after-sales services for further information at bioreagent@bertinpharma.com





European patent # 89 139 552 U.S. patent # 50 47 330

Acylated Ghrelin (dog) Easy Sampling Enzyme Immunoassay kit #A05321.96 wells

For research laboratory use only Not for human diagnostic use

This assay has been developed & validated by Bertin Pharma



Version: 0117 Ref. #A11321

Table of contents

Precaution for use	6
▶ Background	7
Principle of the assay	10
Materials and equipment required	12
Sample collection and preparation	13
Reagent preparation	16
Assay procedure	19
Data analysis	25
Acceptable range	26
Typical results	27
Assay validation and characteristics	29
Troubleshooting	39
Bibliography	41

96 wells Storage: -20°C

Expiry date: stated on the package

This kit contains:

	Colour of cap	Item #	Quantity per kit	Form
Strip 96 well Microtiter plate, pre-coated with anti-Ghrelin mouse monoclonal antibody Easy Sampling	Blister with zip	A08306.1 ea	1	-
Acylated Ghrelin Tracer Easy Sampling	Green	A04306.100 dtn	_ 1	Lyophilised
Acylated Ghrelin (dog) Standard	Blue with red septum	A06321.1 ea	2	Lyophilised
Acylated Ghrelin (dog) Quality Control	Green with red septum	A10321.1 ea	2	Lyophilised
Acylated Ghrelin EIA Buffer	Blue	A07106.1 ea	1	Lyophilised
Wash Buffer concentrated 400x	Silver	A17000.1 ea	1	Liquid
Tween 20	Transparent	A12000.1 ea	1	Liquid
Ellman's reagent 49+1	Black with red septum	A09000_49+1. 100 dtn	2	Lyophilised
Technical booklet	-	A11321	1	-
Well cover sheet	-	-	1	

Each kit contains sufficient reagents for 96 wells. This allows for the construction of one standard curve in duplicate and the assay of 36 samples in duplicate.

If you want to use the kit in two times, we provide one additional vial of Standard, one of Quality Control and one of Ellman's Reagent.

Precaution for use

Users are recommended to read all instructions for use before starting work.

Each time a new pipette tip is used, aspirate a sample or reagent and expel it back into the same vessel. Repeat this operation two or three times before distribution in order to equilibrate the pipette tip.

- For research laboratory use only
- > Not for human diagnostic use
- Do not pipet liquids by mouth
- Do not use kit components beyond the expiration date
- Do not eat, drink or smoke in area in which kit reagents are handled
- > Avoid splashing

Wearing gloves, laboratory coat and glasses is recommended when assaying kit materials and samples.

Temperature

Unless otherwise specified, all the experiments are done at room temperature (RT), that is around +20°C. Working at +25°C or more affects the assay and decreases its efficiency.

Background

▶ Acetylcholinesterase AChE® Technology

Acetylcholinesterase (AChE®), the enzymatic label for EIA, has the fastest turnover rate of any enzymatic label. This specific AChE is extracted from the electric organ of the electric eel, *Electrophorus electricus*, and is capable of massive catalytic turnover during the generation of the electrochemical discharges. The use of AChE as enzymatic label for EIA has been patented by the French academic research Institute CEA *[1, 2, 3]*, and Bertin Pharma, formerly known as SPI-Bio, has expertise to develop and produce EIA kits using this technology.

AChE® assays are revealed with Ellman's Reagent, which contains acetylthiocholine as a substrate. The final product of the enzymatic reaction (5-thio-2-nitrobenzoic acid) is bright yellow and can be read at 405-414 nm. AChE® offers several advantages compared to enzymes conventionally used in EIAs:

- > Kinetic superiority and high sensitivity: AChE® shows true first-order kinetics with a turnover of 64,000 sec-1. That is nearly 3 times faster than Horseradish Peroxidase (HRP) or alkaline phosphatase. AChE® allows a greater sensitivity than other labeling enzymes.
- > Low background: non-enzymatic hydrolysis of acetylthiocholine in buffer is essentially absent. So, AChE® allows a very low background and an increased signal/noise ratio compared to other substrate of enzymes which is inherently unstable.

- Wide dynamic range: AChE® is a stable enzyme and its activity remains constant for many hours as, unlike other enzymes, its substrate is not suicidal. This permits simultaneous assays of high diluted and very concentrated samples.
- > Versatility: AChE® is a completely stable enzyme, unlike peroxidase which is suicidal. Thus, if a plate is accidentally dropped after dispatch of the AChE® substrate (Ellman's Reagent) or if it needs to be revealed again, one only needs to wash the plate, add fresh Ellman's Reagent and proceed with a new development. Otherwise, the plate can be stored at +4°C with Wash Buffer in wells while waiting for technical advice from the Bioreagent Department.

Ghrelin

Ghrelin discovered in 1999, is fast becoming an endocrinology target of the millennium. Ghrelin, identified in rat stomach as an endogenous ligand for the GH secretagogue receptor, is mainly produced in stomach, but has been demonstrated in many other organs [4, 5].

In addition to GH-releasing properties and its orexant action, Ghrelin could act as an hormone having effects on gastric motility (similarity with the peptide hormone motilin), acidic secretion, cardiovascular action, antiproliferative effects, pancreatic and glucose metabolism function, sleep [6, 7, 8]...

Ghrelin gene raises to mRNA prepro-ghrelin of 117 amino acids. This precursor is processed into Ghrelin, 28 amino acids (human).

Before being secreted, this peptide is octanoylated at Ser 3 by GOAT (Ghrelin Octanoyl Acyl Transferase). This step is essential for biological activity making GOAT a perfect target for drugs in feeding behaviour. Interestingly, the potential therapeutic importance of this hormone is not restricted to regulation of food intake [9] but also in cachexia (related to cancer treatment, anorexia nervosa or ischemia) [10] gastric motility and may be involved in osteoporosis, somatopause, infertility and ovulation induction, neurological disorders (Alcoholism, Post Traumatic Stress disorders...) [11] and cardiovascular diseases.

Principle of the assay

This Enzyme Immunometric Assay (EIA) is based on a double-antibody sandwich technique. The wells of the plate supplied are coated with a monoclonal antibody specific to the C-terminal part of Ghrelin.

This antibody will bind to any Ghrelin introduced into the wells (standard or sample). After a washing step, the acetylcholinesterase (AChE) - Fab' conjugate (Tracer) which recognises the N-terminal part of Acylated Ghrelin is then added to the wells.

The two antibodies then form a sandwich by binding on different parts of the Acylated Ghrelin.


The sandwich is immobilised on the plate so reagents in excess may be washed away.

The concentration of Acylated Ghrelin (dog) is determined by measuring the enzymatic activity of immobilized Tracer using Ellman's Reagent. AChE Tracer acts on Ellman's Reagent to form a yellow compound that strongly absorbs at 414 nm.

The intensity of the colour, which is determined by spectrophotometry, is proportional to the amount of Acylated Ghrelin (dog) present in the well during the immunological incubation.

This EIA so called Easy Sampling EIA kit works with any sample collected on any kind of protease inhibitors, without extraction but a simple dilution.

The principle of the assay is summarised below:

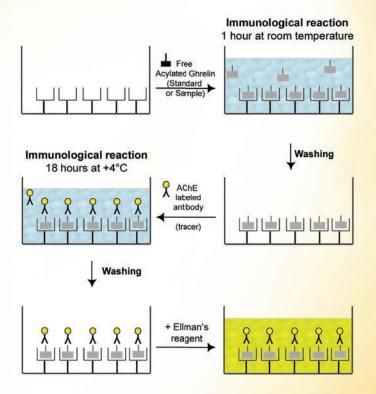

Materials and equipment required

In addition to standard laboratory equipment, the following material is required.

For the sample preparation

- EDTA tubes for blood collection.
- Protease inhibitor (AEBSF, PMSF, Aprotinin, Pefabloc®, P800, PHMB ...)
- VItraPure water #A07001

For the assay

- Precision micropipettes (20 to 1000 μL)
- > Spectrophotometer plate reader (405 or 414 nm filter)
- Microplate washer (or washbottles)
- > Orbital microplate shaker able to perform at 600 rpm
- > Multichannel pipette and disposable tips 30-300 μL
- > UltraPure water (Ref. #A07001)
- > Polypropylene tubes



Water used to prepare all EIA reagents and buffers must be UltraPure (deionized & free from organic contaminant traces).

Otherwise, organic contamination can significantly affect the enzymatic activity of the tracer Acetylcholinesterase (AChE).

Do not use distilled water, HPLC-grade water or sterile water.

UltraPure water may be purchased from Bertin Pharma: item #A07001.1L

Sample collection and preparation

This assay has been validated to measure Acylated Ghrelin in blood and plasma samples (see validation data at the end of this booklet).

General precautions

- All samples must be free of organic solvents prior to assay.
- Samples should be assayed immediately after collection or should be stored at -20°C.

Blood collection

Blood samples are collected in tubes containing EDTA and a protease inhibitor to prevent the degradation of Acylated Ghrelin.

Choice of protease inhibitor

We suggest adding AEBSF at 0.2 mg/mL blood during blood collection.

We suggest preparing a 100 times concentrated solution of protease inhibitor and then adding 10 μ L of this solution per mL of blood. For example, for the AEBSF, prepare a mother solution at 20 mg/mL in UltraPure water and add 10 μ L of this solution per mL of blood. The mother solution may be stored one month at -20°C. We suggest using aliquots for AEBSF solution in order to avoid freezing/thawing cycles.

for later use.

Other protease inhibitors could be used with the assay like Aprotinin (up to 0,6 TIU/mL blood), PMSF (around 0.1 mg/mL blood according to literature), PHMB, Pefabloc® or Pefabloc SC® (up to 0.2 mg/mL blood) as indicated in the section "Protease inhibitor compatibility table" at the end of this booklet. For the use of these different products, please refer to the vendor's instructions.

Collection tubes are mixed by inversion 5 folds.



Samples should be kept on ice between collection and centrifugation (15 minutes max).

- Blood samples are centrifuged at 3,500 rpm for 10 minutes at +4°C and then, supernatants are transferred in separate tubes.
 Samples should be quickly assayed or stored at -20°C
- > The best way is to assay the samples within 3 weeks after the collection date. Moreover, we suggest using aliquots for plasma samples (we suggest 250 µl per aliquot) in order to avoid freezing/thawing cycles.



Plasma samples prepared as above-mentioned can be assayed for Acylated Ghrelin with Acylated Ghrelin Easy Sampling EIA kit or for Unacylated Ghrelin with Unacylated Ghrelin Easy Sampling EIA kit.

Sample preparation

Plasma samples may be assayed directly without any extraction procedure after being diluted at least to 1:5 in EIA Buffer in order to avoid matrix effect.

Reagent preparation

Each kit contains sufficient reagents for 96 wells. This allows for the construction of one standard curve in duplicate and the assay of 36 samples in duplicate.

If you want to use the kit in two times, we provide one additional vial of Standard, one of Quality Control and one of Ellman's Reagent.

All reagents need to be brought to room temperature, around +20°C, prior to the assay.

EIA Buffer

Reconstitute the vial #A07106 with 50 mL of UltraPure water. Allow it to stand 5 minutes until completely dissolved and then mix thoroughly by gentle inversion.

Stability at 4°C: 1 month

Acylated Ghrelin (dog) Standard

Reconstitute the Standard vial #A06321 with 1 mL of UltraPure water. Allow it to stand 5 minutes until completely dissolved and then mix thoroughly by gentle inversion.

The concentration of the first standard S1 is 250 pg/mL.

Prepare seven propylene tubes for the other standards and add 500 μ L of EIA Buffer into each tube. Then prepare the standards by serial dilutions as follows:

Standard	Volume of Standard	Volume of EIA Buffer	Standard concentration pg/mL
S1	-	-	250
S2	500 μL of S1	500 μL	125
S3	500 μL of S2	500 μL	62.5
S4	500 μL of S3	500 μL	31.3
S5	500 μL of S4	500 μL	15.6
S6	500 μL of S5	500 μL	7.8
S7	500 μL of S6	500 μL	3.9
S8	500 μL of S7	500 μL	2.0

Stability at 4°C: 1 week

Acylated Ghrelin (dog) Quality Control

The Quality Control provided in this kit has been prepared by spiking Acylated Ghrelin (dog) peptide in EIA Buffer.

Reconstitute the Quality Control vial #A10321 with 1 mL of UltraPure water. Allow it to stand 5 minutes until completely dissolved and then mix thoroughly by gentle inversion.

Stability at +4°C: 1 week

Acylated Ghrelin Tracer Easy Sampling

Reconstitute the vial #A04306 with 10 mL of EIA Buffer. Allow it to stand 5 minutes until completely dissolved and then mix thoroughly by gentle inversion.

Stability at +4°C: 1 week

Wash Buffer

Dilute 2 mL of concentrated Wash Buffer #A17000 with 800 mL of UltraPure water. Add 400 µL of Tween20 #A12000. Use a magnetic stirring bar to mix the content.

Stability at +4°C: 1 week

Ellman's Reagent

5 minutes before use (development of the plate), reconstitute one vial of Ellman's Reagent #A09000_49+1 with 49 mL of UltraPure water and 1 mL of concentrated Wash Buffer. The tube content should be thoroughly mixed.

Stability at 4°C and in the dark: 24 hours

Assay procedure

It is recommended to perform the assays in duplicate and to follow the instructions hereafter.

Plate preparation

Prepare the Wash Buffer as indicated in the reagent preparation section.

Open the plate packet and select the sufficient strips for your assay and place the unused strips back in the packet. Stability at $+4^{\circ}C$: 1 month.


Rinse each well 5 times with the Wash Buffer 300 µL/well.

Just before distributing reagents and samples, remove the buffer from the wells by inverting the plate and shaking out the last drops on a paper towel.

Plate set-up

A plate set-up is suggested hereafter.

The contents of each well may be recorded on the template sheet provided at the end of this technical booklet.

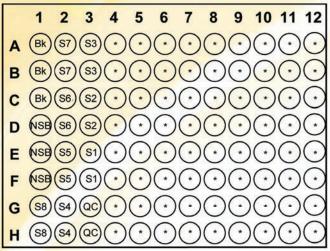

Bk: Blank S1-S8: Standards 1-8
NSB: Non Specific Binding QC: Quality Control

* : Samples

Pipetting the reagents

All samples and reagents must reach room temperature prior to performing the assay.

Use different tips to pipette the Buffer, Standard, Sample, Tracer and other reagents.

Before pipetting, equilibrate the pipette tips in each reagent. Do not touch the liquid already in the well when expeling with the pipette tip.

> EIA Buffer

Dispense 100 µL to Non Specific Binding NSB wells.

> Acylated Ghrelin (dog) Standards

Dispense 100 μL of each of the eight standards S1 to S8 in duplicate to appropriate wells.

Start with the lowest concentration standard S8 and equilibrate the tip in the next higher standard before pipetting.

Quality Control and samples

Dispense 100 µL in duplicate to appropriate wells. Highly concentrated samples may be diluted in EIA Buffer.

Incubating the plate

Cover the plate with the cover sheet and incubate for 1 hour at room temperature on an orbital shaker (at 600 rpm).

Technical note

This kit was validated with two incubation steps: 1 hour RT + overnight at $+4^{\circ}C$; but it works as well with two incubation steps: 2 hours RT + 2 hours RT on an orbital shaker.

Washing the plate

Empty the plate by turning over. Rinse each well five times with 300 µL Wash Buffer. The 5th time, slightly shake the plate for 5 minutes on an orbital shaker. Then rewash five times with 300 µL Wash Buffer.

At the end of the last washing step, empty the plate and blot the plate on a paper towel to discard any trace of liquid.

Pipetting the reagents

> Acylated Ghrelin Tracer
Dispense 100 µL to each well, except blank (Bk) wells.

Incubating the plate

Cover the plate with the cover sheet and incubate overnight (18 to 20 hours) at +4°C.

Technical note

This kit was validated with two incubation steps: 1 hour RT + overnight at $+4^{\circ}$ C; but it works as well with two incubation steps: 2 hours RT + 2 hours RT on an orbital shaker.

Developing and reading the plate

Reconstitute Ellman's reagent as mentioned in the Reagent preparation section.

- > Empty the plate by turning over. Rinse each well five times with 300 µL Wash Buffer. The 5th time, slightly shake the plate for 5 minutes on an orbital shaker. Then rewash five times with 300 µL Wash Buffer. At the end of the last washing step, empty the plate and blot the plate on a paper towel to discard any trace of liquid.
- Add 200µL of Ellman's reagent to each 96 well. Cover the plate with aluminium sheet and incubate in the dark at room temperature. Optimal development is obtained using an orbital shaker.
- > Wipe the bottom of the plate with a paper towel, and make sure that no liquid has splashed outside the wells.
- Read the plate at a wavelength between 405 and 414nm (yellow colour).

After addition of Ellman's reagent, the absorbance has to be checked periodically (every 30 minutes) until the maximum absorbance has reached a minimum of 0.5 A.U. blank subtracted.

Easy Sampling	g Enzyme Immu	unoassay Proto	cole (volumes a	ıre in μL)			
Volume Wells	Blank	NSB	Standard	Sample or QC			
EIA Buffer	EIA Buffer - 100						
Standard	- 100 -						
Sample or QC 100							
Cover plate, incubate 1 hour at 600 rpm at RT							
Wash plate 5 times, shake 5 min, wash 5 times & discard liquid from the wells							
Tracer	Tracer - 100 100 100						
	Cover plate, ir	cubate overnight	at +4°C				
Wash plate 5 times, shake 5 min, wash 5 times & discard liquid from the wells							
Ellman's reagent 200							
Ir	cubate with an o	rbital shaker in t	he dark at RT	Eirin			
	Read the plate	between 405 and	d 414 nm				

Data analysis

Make sure that your plate reader has subtracted the absorbance readings of the blank well (absorbance of Ellman's reagent alone) from the absorbance readings of the rest of the plate. If not, do it now.

- Calculate the average absorbance for each NSB, standard and sample.
- For each standard, plot the absorbance on y axis versus the concentration on x axis. Draw a best-fit line through the points.
- > To determine the concentration of your samples, find the absorbance value of each sample on the y axis.
- Read the corresponding value on the x axis which is the concentration of your unknown sample. Do not forget to integrate the dilution factor of your own samples (due notably to the minimal dilution for the assay 1:2).
- Samples with a concentration greater than 250 pg/mL should be re-assayed after dilution in EIA Buffer.
- Most plate readers are supplied with curve-fitting software capable of graphing these data (logit/log or 4-parameter logistic fit 4PL). If you have this type of software, we recommend using it. Refer to it for further information.



Two vials of Quality Control are provided with this kit.

Your standard curve is validated only if the calculated concentration of the Quality Control obtained with the assay is +/- 25% of the expected concentration (see the label of QC vial)

Acceptable range

- Non Specific Binding < 50 mA.U.</p>
- Limit of detection in sample before dilution <10 pg/mL</p>
- > QC sample: ±25% of the expected concentration (see the label of QC vial)


Typical results

The following data are for demonstration purpose only. Your data may be different and still correct.

These data were obtained using all reagents as supplied in this kit under the following conditions: 60 minutes developping, reading at 405 nm. A 5-parameter logistic fitting with ponderation 1/Y2 was used to determine the concentrations.

	Acylated Ghrelin (dog) pg/mL	Absorbance (mAU)
Standard S1	250	1900
Standard S2	125	1154
Standard S3	62.5	585
Standard S4	31.3	319
Standard S5	15.6	158
Standard S6	7.8	87
Standard S7	3.9	52
Standard S8	2.0	34
Blank	0	10

Typical Acylated Ghrelin (dog) Easy Sampling standard curve

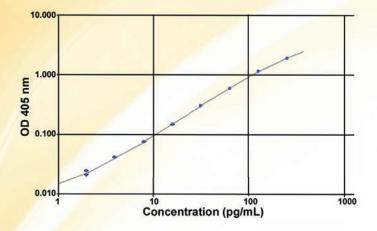

Assay validation and characteristics

The Enzyme Immunometric assay of Acylated Ghrelin (dog) has been validated for its use in buffer and in plasma (without extraction but diluted at least 1:5). A 5-parameter logistic fitting with ponderation 1/Y2 was used to determine the concentrations.

For additional information regarding the validation of imunoassay for protein biomarkers in biological samples, please refer to bibliography *[12, 13]*.

- > The **limit of detection**, calculated as the concentration of Acylated Ghrelin corresponding to the NSB average (n = 8) plus three standard deviations is 2 pg/mL. Due to the minimal plasma dilution (1:5), the limit of detection in the samples is 10 pg/mL.
- Intra-assay & inter-assay variations and recovery

	Inte	r-assay		Intra-assay		
QC levels after 1:5 dilution (pg/mL)	Mean of observed concentrations (pg/mL)	cv (%)	Recovery (%)	Mean of observed concentrations (pg/mL)	cv (%)	Recovery (%)
200 (ULOQ)	227.0	7.66	13.3	235.0	4.89	17.3
150 (HQC)	160.0	4.00	6.8	168.0	2.16	12.3
50 (MQC)	49.4	7.44	-1.2	50.3	2.81	0.5
10 (LQC)	9.9	9.50	-1.0	10.2	3.24	1.7
5 (LLOQ)	5.1	9.00	-2.5	5.0	2.85	0.0

ULOQ: Upper Limit of Quantification

HQC: High QCMQC: Mid QC

LOC: Low OC

LLOQ: Lower Limit of Quantification

The intra-assay and inter-assay variations were studied on a pool of dog plasma containing AEBSF 0.4 mg/mL (free of Ghrelin) spiked samples for each level of QC. QC were prepared five times concentrated from a pool of dog plasma and then diluted to 1:5 in EIA Buffer before assay.

For within-run precision and accuracy, the number of replicates (n) is equal to 6 for each levels of QC, the five QC samples were analysed along with the calibration curve for a unique experiment.

For between-run precision and accuracy, the number of replicates (n) is equal to 6 for each levels of QC, the five QC samples were analysed along with the calibration curve for a total of 6 independent experiments.

> Selectivity

Matrix	Mean of measured concentration (pg/mL)	CV (%)	Recovery (%)
1	3.71	7.59	-25.8
2	3.93	0.01	-21.3
3	3.80	4.50	-24.0
4	3.45	2.50	-31.1
5 (haemolysed)	3.91	2.18	-21.7
6	4.93	2.87	-1.48
7	3.47	6.59	-30.5
8	4.19	4.91	-16.3
9	2.89	17.8	-42.3
10 (haemolysed)	3.14	6.06	-37.2

Selectivity was tested by spiking 10 sources of samples matrix containing AEBSF at 0.4 mg/mL at the LLOQ (n=3).

These sources included 2 haemolysed samples (matrix 5 and 10). QC samples (n=3) were prepared five times concentrated in each matrix (free of Ghrelin) and then diluted to 1:5 in EIA buffer in order to obtain a final concentration of 5 pg/mL and analysed against a calibration curve.

> Specificity

Specificity was tested by adding AEBSF at 0.4 mg/mL (recommended use concentration for blood collection) and 2 mg/mL (high concentration) or aprotinin at 1.2 TIU/mL with or without HCl 0.1 N final into sample matrix (a pool of dog plasma samples) and measuring the accuracy of the Acylated Ghrelin (dog) at both LLOQ and ULOQ (n=3).

Matrix	QC level after 1:15 dilution (pg/mL)	Mean of measured concentration (pg/mL)	CV (%)	Recovery (%)
AFRSE O 4 mm/ml	5	4.28	1.96	-14.4
AEBSF 0.4 mg/mL	200	208	7.68	3.9
AEBSF 0.4 mg/mL	5	4.33	2.64	-13.3
+ HCI 0.1N	200	211	2.48	5.3
AFRCE 2 may/ml	5	4.57	4.23	-8.6
AEBSF 2 mg/mL	200	230	3.67	14.8
AEBSF 2 mg/mL	5	5.11	2.29	2.3
+ HCI 0.1N	200	223	2.81	11.4
Association 1 2 THI/pol	5	3.37	5.83	-32.7
Aprotinin 1.2 TIU/mL	200	176	2.76	-11.9
Aprotinin 1.2 TIU/mL	5	3.63	3.82	-27.5
+ HCI 0.1N	200	185	1.25	-7.3

Dilution tests

Dilution linearity was tested by spiking a pool of dog plasma samples (free of Ghrelin) containing AEBSF at 0.4 mg/mL at 2000 pg/mL (n=3) and measuring precision and accuracy after serial dilution in EIA buffer to bring the AG concentrations into the validated range for analysis (between ULOQ and LLOQ).

Dilution factor	Theoretical concentration (pg/mL)	Measured con- centration (pg/mL)	Corrected concentration (ng/mL)	Recovery (%)	Mean recovery (%)	%AO
		192	1920	-4.0		
1:10	200	171	1710	-14.5	-8.2	
		188	1880	-6.0		
		90.4	1808	9.6-		
1:20	100	87.2	1744	-12.8	-12.6	
		84.6	1692	-15.4		
		46.7	1868	9.9-		
1:40	20	42.8	1712	-14.4	-12.3	5.19
		42.1	1684	-15.8		
		23.8	1904	-4.8		
1:80	25	21.3	1704	-14.8	-10.9	
		21.7	1736	-13.2		
		12.1	1936	-3.2		
1:160	12.5	10.6	1696	-15.2	6.6-	
		11.1	1776	-11.2		

> Parallelism

Parallelism between the calibration standard curve and serial diluted samples was tested by diluting 3 samples containing AEBSF at 0.4 mg/mL in EIA buffer (n=3) to bring the Acylated Ghrelin concentrations into the validated range for analysis (between ULOQ and LLOQ).

Sample	Dilution series	Dilution factor	Measured concentration (pg/mL)	Corrected concentration (pg/mL)	CV (%)
		1:5	50.0	250	
	1	1:10	23.9	239	9.88
		1:20	10.3	206	=
		1:5	50.2	251	
1	2	1:10	23.8	238	4.83
		1:20	11.4	228	
		1:5	49.2	246	
	3	1:10	23.7	237	2.61
		1:20	11.7	234	
		1:2	65.4	327	
	1	1:5	28.0	280	9.88
		1:10	13.7	274	
		1:2	62.8	314	
2	2	1:5	29.6	296	8.30
		1:10	13.3	266	
		1:2	64.3	322	
	3	1:5	30.9	309	5.17
		1:10	14.5	290	

Sample	Dilution series	Dilution factor	Measured concentration (pg/mL)	Corrected concentration (pg/mL)	CV (%)
		1:2	46.0	230	
	1	1:5	21.6	216	5.11
		1:10	10.4	208	
		1:2	47.9	240	
3	2	1:5	20.5	205	11.30
		1:10	9.7	193	
		1:2	44.4	222	
	3	1:5	20.7	207	9.37
		1:10	9.2	184	

Stability test (freezing/thawing, 24h at +5°C and 24h at +20/+25°C)

Stability of Aylated Ghrelin was evaluated by using samples of the Low and High level QC samples. These QC samples (n=3) were prepared in a pool of dog plasma (free of Ghrelin) containing AEBSF at 0.4 mg/mL or aprotinin at 1.2 TIU/mL and then frozen at -20°C for freeze/thaw stability or stored 24h at +5°C or 20-25°C for short-term stability.

Conditions	QC level after 1:5 dilution (pg/mL)	Mean of measured concentration (pg/mL)	CV (%)	Recovery (%)
Freeze/thaw	10	9.32	2.63	-6.8
1 cycle AEBSF 0.4 mg/mL	150	150	2.40	0.3
Freeze/thaw	10	8.28	1.26	-17.2
3 cycles AEBSF 0.4 mg/mL	150	136	3.56	-9.1
Freeze/thaw	10	8.46	3.25	-15.4
1 cycle Aprotinin 1.2 TIU/mL	150	134	3.38	-10.4
Freeze/thaw	10	7.21	3.36	-28.0
3 cycles Aprotinin 1.2TIU/mL	150	124	2.07	-17.2
24h at +5°C	10	7.81	4.45	-21.9
AEBSF 0.4 mg/mL	150	125	1.61	-16.6
24h at 20-25°C	10	9.95	2.35	-0.5
AEBSF 0.4 mg/mL	150	158	4.30	5.2

Cross-reactivity

Acylated Ghrelin (human)	120%	
Acylated Ghrelin (rat)	120%	
Unacylated Ghrelin (dog)	<1%	
Unacylated Ghrelin (rat)	<1 %	
Unacylated Ghrelin (human)	<1%	
Ghrelin (1-14) (human)	<0.001 %	
Ghrelin (1-11) (rat)	<0.001 %	
Ghrelin (17-28) (human, rat)	<0.001 %	
GHRF (human)	<0.001 %	
Insulin (human)	<0.001 %	
Motiline	<0.001 %	
Leptin (human)	<0.001 %	
Somatostatine	<0.001 %	
CRF (human, rat)	<0.001 %	
Glucagon (human, rat)	<0.001 %	

> Protease Inhibitor compatibility table

	AEBSF	PMSF	Pefabloc	P800	Aprotinin	PHMB
A05321.96 wells	YES	YES	YES	YES	YES	YES

Plasma samples were collected on different protease inhibitors according to vendors instruction and measured with the appropriate kit. Recovery is different from one inhibitor to the other and it belongs to the end user to define according to its needs which inhibitor to be used. Acidification has also been tested with most inhibitors and may also change recovery, but will not affect the assays performances providing that 1:5 dilution with EIA Buffer or neutralisation is performed.

> Related products

Item Reference	Designation	Application		
A05106.96 wells	Acylated Ghrelin (human) Express EIA kit	PHMB, PMSF, Aprotinin samples		
A05106.384 wells	Acylated Ghrelin (human) 384w EIA kit	GOAT inhibitor screening		
A05117.96 wells	Acylated Ghrelin (mouse, rat) Express EIA kit	PHMB, PMSF, Aprotinin samples		
A05118.96 wells	UnAcylated Ghrelin (mouse, rat) Express EIA kit	PHMB, PMSF, Aprotinin samples		
A05119.96 wells	UnAcylated Ghrelin (human) Express EIA kit	PHMB, PMSF, Aprotinin samples		
A05306.96 wells	Acylated Ghrelin (human) Easy Sampling EIA kit	Any kind of sample		
A05317.96 wells	Acylated Ghrelin (mouse, rat) Easy Sampling EIA kit			
A05318.96 wells	UnAcylated Ghrelin (mouse, rat) Easy sampling EIA kit			
A05319.96 wells	UnAcylated Ghrelin (human) Easy Sampling EIA kit			
A05320.96 wells	UnAcylated Ghrelin (dog) Easy Sampling EIA kit			
A05321.96 wells	Acylated Ghrelin (dog) Easy Sampling EIA Kit			
A05401.96 wells	Acylated Ghrelin (pig) EIA kit	PHMB, PMSF, Aprotinin samples		
A05402.96 wells	UnAcylated Ghrelin (pig) EIA kit	PHMB, PMSF, Aprotinin samples		
D31009	Sampling Tubes with PHMB	Sample preparation		

Troubleshooting

- Absorbance values are too low:
 - organic contamination of water,
 - one reagent has not been dispensed,
 - incorrect preparation/dilution,
 - assay performed before reagents reached room temperature,
 - reading time not long enough.

High signal and background in all wells:

- inefficient washing,
- overdeveloping (incubation time should be reduced),
- high ambient temperature.

> High dispersion of duplicates:

- poor pipetting technique,
- irregular plate washing.
- If a plate is accidentally dropped after dispatch of the AChE® substrate (Ellman's Reagent) or if it needs to be revealed again:
 - one only needs to wash the plate, add fresh Ellman's Reagent and proceed with a new development.
 - otherwise, the plate can be stored at +4°C with Wash Buffer in wells while waiting for technical advice from the Bioreagent Department.

These are a few examples of trouble shooting that may occur.

If you need further explanation, Bertin Pharma will be happy to assist you. Feel free to contact our technical support staff by phone (+33 (0)139 306 036), fax (+33 (0)139 306 299) or E-mail (bioreagent@bertinpharma.com), and be sure to indicate the batch number of the kit (see outside the box).

Bertin Pharma proposes EIA Training kit #B05005 and EIA workshop upon request. For further information, please contact our Marketing Department by phone (+33 (0)139 306 260) or E-mail (marketing@bertinpharma.com).

Bibliography

Grassi J., Pradelles P.

Compounds labelled by the acetylcholinesterase of *Electrophorus Electricus*. Its preparation process and its use as a tracer or marquer in enzymo-immunological determinations. *United States patent, N° 1,047,330. September 10, 1991*

Grassi J., Pradelles P.

The use of Acetylcholinesterase as a Universal marker in Enzyme-Immunoassays

Proceedings of the Third International Meeting on

Cholinesterases, American Chemical Society (1991)

Pradelles P., Grassi J. and Maclouf J.
 Enzyme Immunoassays of Eicosanoids Using Acetylcholinesterase.

 Methods in Enzymology (1990), vol. 187, 24-34

Kojima M., Kangawa K.
 Ghrelin: structure and function
 Physiol. Rev (2005), 85:495-522,

- Bluet-Pajot M-T., Tolle V., Zizzari P., et al.
 Ghrelin: A striking example of neuroendocrine peptide pleiotropy Med Sci (Paris), August 1, 2005, 21 (8-9): 715-21
- de Faria Barros A. et al.
 Is there association between acyl-ghrelin and inflammation in hemodialysis patients?
 J Bras Nefrol. (2013) 35(2):120-126.

7. Grousselle D. et al.

Variations des peptides dérivés de la préproghréline au cours du repas dans l'anorexie mentale restrictive

Poster GIR-AFDAS-TCA2014

8. Delhanty P. et al.

Des-acyl ghrelin analogs prevent high-fat-diet-induced dysregulation of glucose homeostasis

FASEB J. (2013) 27(4):1690-1700.

9. Costantini V. et al.

GSK1614343, a Novel Ghrelin Receptor Antagonist, Produces an Unexpected Increase of Food Intake and Body Weight in Rodents and Dogs

Neuroendocrinology (2011); 94: 158–168

10. Porporato E., Filigheddu N. et al.

Acylated and unAcylated Ghrelin impair skeletal muscle atrophy in mice.

J. Clinical Invest (2013) 123(2): 611-622

Sentissi O., Epelbaum J., Olié J-P. et al.
 Leptin and Ghrelin Levels in Patients With Schizophrenia During
 Different Antipsychotics Treatment: A Review
 Schizophrenia Bulletin (2008) 34(6), 1189–1199

12. Valentin M-A., Ma S., Zhao A. et al.

Validation of immunoassay for protein biomarkers: Bioanalytical study plan implementation to support pre-clinical and clinical studies.

J Pharm Biomed Anal. (2011) 55(5): 869-877

13. European Medicines Agency

Guideline on bioanalytical method validation, 21 July 2011

Additional readings


List of publications quoting the use of SPI-Bio Ghrelin kits

14. Delhanty P. et al.

The Acylated (AG) to Unacylated (UAG) Ghrelin Ratio in Esterase Inhibitor Treated Blood Is Higher Than Previously Described Poster SUN-1060, 16th International Congress of Endocrinology ICE ENDO 2014 June 2014.

[&]quot;This document is copyrighted. All rights are reserved. This document may not, in whole or part, be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine readable form without the prior consent, in writing, from Bertin Pharma."

A05321 - Acylated Ghrelin (dog) Easy Sampling

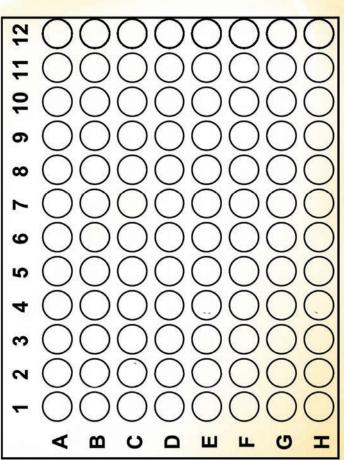



A05321 - Acylated Ghrelin (dog) Easy Sampling

Bertin Pharma, over the last decades, has been developing and marketing over 100 biomarker assays, pre-analytical products, kits, antibodies and biochemicals thanks to its innovative work in research and development. Our core areas are orientated to inflammation, oxidative injury, endocrinology, diabetes, obesity, hypertension, neurodegenerative diseases, HIV, prion diseases, pharmacokinetics and metabolism.

Bertin Pharma is active worldwide either with direct sales or through our qualified and trained international distribution network from the United States to Japan.

We are able to provide you with local technical support to use at ease our products.

For further information, please send your request to bioreagent@bertinpharma.com

